

HIGH SENSITIVITY HUMAN SOLUBLE CD25 /IL-2RA ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF
HUMAN SOLUBLE CD25 /IL-2 RECEPTOR ALPHA
CONCENTRATIONS IN PLASMA AND SERUM



ALWAYS REFER TO LOT SPECIFIC PROTOCOL
PROVIDED WITH EACH KIT FOR
INSTRUCTIONS. PROTOCOL MUST BE
READ AND CHECK ALL ITEMS OF EACH KIT
BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN
DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

THIS IS FOR ONE TIME USE ONLY

ELISA NAME	HUMAN SOLUBLE CD25/IL-2RA ELISA KIT
Catalog No.	SK00761-06
Formulation	96 T
Lot No.	
Standard range	4.8 ~ 625 pg/mL
Sensitivity	3 pg/mL
Sample Volume	100 µL
Dilution Factor	Optimal dilutions should be determined by each laboratory for each application
Sample Type	Serum, Plasma, Cell Cultures
Specificity	Human soluble CD25/IL-2RA
Calibration	Human Soluble CD25 His Tag (HEK293)
Intra-assay Precision	4 - 6%
Inter-assay Precision	4 - 8%
Storage	2 – 8 °C for 1 month. See detail on page 2-3
This kit contains sufficient materials to run 35-40 samples duplicated provided that assay is run according to protocol.	

Order Contact:

AVISCERA BIOSCIENCE, INC.

2348 Walsh Ave., Suite C

Santa Clara, CA 95051

Tel: (408) 982 0300

Email: Sales@AvisceraBioscience.com

Info@AvisceraBioscience.com

www.AvisceraBioscience.com

www.AvisceraBioscience.net

DESCRIPTION

This High Sensitivity Human Soluble CD25 /IL-2RA ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural human soluble CD25 from serum and plasma in a sandwich ELISA format.

This immunoassay contains recombinant human soluble CD25 derived from HEK293 and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural the soluble CD25 samples.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with a monoclonal antibody specific for human CD25. The capture antibody can bind to the human soluble CD25 in the standard and samples. After washing the plate of any unbound substances, a biotinylated antibody against human soluble CD25 is added to the wells. After another washing of the plate, the streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution (TMB) is added to the wells and color develops in direct proportion to the amount of human the soluble CD25 bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

DESCRIPTION	CODE	QUANTITY
sCD25 Microplate – 96 well microplate coated with monoclonal antibody specific for human soluble CD25.	761-06-01	1 plate
sCD25 Standard – refer to lot specific of lyophilized recombinant human soluble CD25 (HEK293).	761-06-02	1 vial
Detection Antibody Concentrate – 1.2 mL/vial of 10-fold concentrate of lyophilized biotinylated antibody against human soluble CD25.	761-06-03	1 vial
Positive Control – one vial of lyophilized recombinant human soluble.	761-01-04	1 vial
Streptavidin-HRP Conjugate – 120 µL/vial of 100-fold concentrated solution of Streptavidin-HRP conjugate.	SAHRP	1 vial
Dilution Buffer – 45 mL of buffered solution with preservative.	DB05	1 bottle
Antibody Diluent Solution – 12 mL of buffered solution with preservative.	DB11C	1 bottle
HRP Diluent Solution – 12 mL of buffered solution with preservative.	DB08B	1 bottle
Wash Buffer – 50 mL of 10-fold concentrated buffered surfactant with preservative.	WB01	1 bottle
TMB Substrate Solution – 11 mL of TMB substrate solution.	TMB01	1 bottle
Stop Solution – 11 mL of 0.25M HCl.	S-STOP	1 bottle
Plate Sealer	EAPS	1 piece
Plastic Pouch	P01	1 piece

STORAGE

Unopened Kit: Store at 2 – 8 °C for up to 1 month. For longer storage for up to 8 months, unopened Standard, Positive Control, Detection Antibody Concentrate, Dilution Buffer and HRP Diluent Solution should be stored at -20 °C or -70 °C. Streptavidin-HRP Conjugate and Substrate Solution should be stored only at 2 – 8 °C. Do not use kit past expiration date.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (350 – 400 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE COLLECTION AND STORAGE

Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Optional: Use Protease Inhibitors (Order No.: PI-00978-50) for ALL sample collection to prevent sample degradation. 10 µL per ml of sample solution.

Optimal dilutions should be determined by each laboratory for each application with a pretest. Use polypropylene test tubes.

REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer – Dilute 50 mL of Wash Buffer Concentrate into 450 mL distilled or deionized water to make 500 mL of 1x Wash Buffer. If crystals have formed in the concentrate, warm bottle in a water bath until the crystals have completely dissolved.

sCD25 Standard – Reconstitute the soluble CD25 standard with refer to lot of Dilution Buffer. Allow the stock standard to sit for at least 15 minutes with gentle agitation until completely dissolved prior to making standard dilutions (see below). Mix each tube thoroughly before the next transfer.

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
Stock	powder	Refer to lot	XXXXX
# 1	Refer to lot	Refer to lot	625 pg/mL
# 2	250µL of 1	250µL	312.5 pg/mL
# 3	250µL of 2	250µL	156.25 pg/mL
# 4	250µL of 3	250µL	78.125 pg/mL
# 5	250µL of 4	250µL	39.063 pg/mL
# 6	250µL of 5	250µL	19.531 pg/mL
# 7	250µL of 6	250µL	9.766 pg/mL
# 8	250µL of 7	250µL	4.883 pg/mL

SAMPLE PREPARATION

Detection Antibody - Reconstitute the Detection Antibody Concentrate with 1.2 mL of **Antibody Diluent Solution** to produce a 10-fold concentrated stock solution. Allow the concentrated solution to sit for at least 5 minutes until completely dissolved. Pipette 9.45 mL of **Antibody Diluent Solution** into a 15 mL centrifuge tube and transfer 1.05 mL of 10-fold concentrated stock solution to prepare working solution.

Streptavidin-HRP Conjugate - Pipette 11.88 mL of HRP Diluent Solution (DB08B) into a 15 mL centrifuge tube and transfer 120 µL of 100-fold concentrated stock solution to prepare working solution. **Note:** 1x working solution of streptavidin-HRP should be used within a few hours (**protect from light**). **DO NOT FREEZE.**

Positive Control - Reconstitute the Positive Control with 1.0 mL Dilution Buffer.

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.

1. Prepare all reagents, standard dilutions, positive control and samples as directed previously.
2. Remove unneeded microplate strips from the plate frame and return them to the plastic pouch with the desiccant pack.
3. Add 100 µL per well of **Dilution Buffer** to Blank wells.
4. Add 100 µL per well of **Standard Dilutions, sample, or positive control**. Cover with plate sealer and incubate for 2 hours on microplate shaker at room temperature. (Please see plate layout provided.)
5. Aspirate and wash each well with 300 µL of **1x Wash Buffer** four times. After the last wash, aspirate any remaining 1x Wash Buffer, invert the plate and blot against clean paper towel(s).
6. Add 100 µL per well of **Detection Antibody working solution**. Cover with plate sealer and incubate for 2 hours on microplate shaker at room temperature.
7. Repeat the aspiration and wash as in step 5.

8. Add 100 µL per well of **Streptavidin-HRP Conjugate working solution**. Cover with plate sealer and incubate for 45 minutes on microplate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration and wash as in step 5.
10. Add 100 µL per well of **Substrate Solution**. Incubate for 5-10 minutes on microplate shaker at room temperature. **Protect from light.**
11. Add 100 µL per well of **Stop Solution**. The color in the wells should change from blue to yellow. If the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Read plate using a microplate reader set to 450 nm within 3 minutes.

CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log or 4-parameter curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

SPECIFICITY

PROTEIN	CROSS-REACTIVITY
Human sIL-2Ra/CD25 (HEK293)	100%
Human IL-2	0
Mouse sCD25	0
Human IL-6R	0
Human IL-6	0

Add 100 μ L per well of Stop Solution. Read at 450 nm within 3 minutes.

TYPICAL STANDARD CURVE


This standard curve is for demonstration only. A new standard curve should be made for each set of samples assayed.

STANDARD (PG/ML)	AVERAGE OD450NM (CORRECTED)
Blank	0 (0.119)
4.8	0.035
9.7	0.071
19.5	0.128
39	0.259
78	0.515
156	1.009
312.5	1.769
625	2.519

Human Soluble IL-2R alpha / CD25 ELISA Kit SK00761-06

Standard Range: 4.8 ~ 625 pg/mL

Sensitivity: 3 pg/mL Calibration: rh CD25 (HEK293)

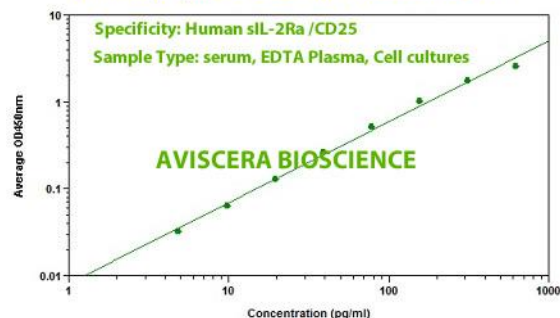

SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARD DILUTIONS
↓
Add 100 μ L of standard dilutions, samples and positive control. Cover with plate sealer and incubate 2 hours on microplate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 μ L per well of Detection Antibody working solution. Cover with plate sealer and incubate 2 hours on microplate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 μ L per well of Streptavidin-HRP Conjugate working solution. Cover with plate sealer and incubate 45 minutes on microplate shaker at RT. Protect from light.
↓
Aspirate and wash 4 times.
↓
Add 100 μ L per well of Substrate Solution. Incubate 5-10 min on microplate shaker at RT. Protect from light.
↓