

MOUSE SOLUBLE SORTILIN ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF MOUSE SOLUBLE SORTILIN CONCENTRATIONS IN CELL CULTURE SUPERNATES AND TISSUE HOMOGENATES



ALWAYS REFER TO LOT SPECIFIC PROTOCOL PROVIDED WITH EACH KIT FOR INSTRUCTIONS. PROTOCOL MUST BE READ BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

ELISA NAME	MOUSE SOLUBLE SORTILIN ELISA
Catalog No.	SK00472-03
Lot No.	20111889
Formulation	96 T
Standard Range	1.56-200 ng/mL
Sensitivity	300 pg/mL
Sample Volume	100 µL
Dilution Factor	Optimal dilutions should be determined by each laboratory for each application
Sample Type	Cell Culture Supernates and Tissue Homogenates
Specificity	Mouse sSortilin
Calibration	sSortilin Recombinant
Intra-assay Precision	4-6%
Inter-assay Precision	8-12%
Storage	2-8°C

This kit contains sufficient materials to run 35 samples duplicated provided that assay is run according to protocol.

Order Contact:

AVISCERA BIOSCIENCE, INC.
2348 Walsh Ave., Suite C
Santa Clara, CA 95051
USA

Tel: (408) 982 0300

Fax: (408) 982 0301

Email: Info@AvisceraBioscience.com

Sales@AvisceraBioscience.com

www.AvisceraBioscience.com

DESCRIPTION

This Mouse Soluble Sortilin (sSortilin) ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural mouse Soluble Sortilin (sSortilin) from cell culture supernates and tissue homogenates in a sandwich ELISA format.

This immunoassay contains recombinant soluble Sortilin (sSortilin) and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural soluble Sortilin (sSortilin) samples.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with an antibody specific for soluble Sortilin (sSortilin). The capture antibody can bind to soluble Sortilin (sSortilin) in the standard and samples. After washing the plate of any unbound substances, a biotinylated antibody against soluble Sortilin (sSortilin) is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution (TMB) is added to the wells and color develops in direct proportion to the amount of soluble Sortilin (sSortilin) bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

DESCRIPTION	CODE	QUANTITY
sSortilin Microplate - 96 well polystyrene microplate (12 strips of 8 wells) coated with an antibody against sSortilin.	472-03-01	1 plate
sSortilin Standard – 200 ng/vial of recombinant sSortilin in a buffered protein base with preservative; lyophilized.	472-03-02	1 vial
Detection Antibody Concentrate – 1.05 mL/vial, 10-fold concentrate of biotinylated antibody against sSortilin with preservative; lyophilized.	472-03-03	1 vial
Positive Control – one vial of recombinant sSortilin; lyophilized.	472-03-04	1 vial
Streptavidin-HRP Conjugate – 120 µL/vial of 100-fold concentrated solution of Streptavidin-HRP with preservative.	SAHRP	1 vial
Dilution Buffer – 60 mL of buffered protein based solution with preservative.	DB08	1 bottle
Wash Buffer - 50 mL of 10-fold concentrated buffered surfactant, with preservative.	WB01	1 bottle
TMB Substrate Solution - 11 mL of TMB Substrate Solution.	TMB01	1 bottle
Stop Solution – 11 mL of 0.5M HCl.	S-STOP	1 bottle
Plate Sealer	EAPS	1 piece
Plastic Pouch	P01	1 piece

STORAGE

Unopened Kit: Store at 2 – 8 °C for up to 8 months. For longer storage, unopened Standard, Positive Control and Detection Antibody Concentrate should be stored at -20 °C or -70 °C. Do not use kit past expiration date.

Opened / Reconstituted Reagents: Reconstituted Standard (stock) solution and Detection Antibody

concentrated solution SHOULD BE STORED at -20 °C or -70 °C for up to one month. Streptavidin-HRP Conjugate 100-fold concentrated solution and TMB Substrate Solution can be stored at 2 – 8 °C for up to 8 months (**DO NOT FREEZE** and **PROTECT FROM LIGHT**). All other components may be stored at 2 – 8 °C for up to 8 months.

Microplate Wells: Return unused strips to the plastic pouch with the desiccant pack. Microplate may be stored for up to 6 months at 2 – 8 °C after opening.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE PREPARATION

Optimal dilutions should be determined by each laboratory for each application with a pretest. Use polypropylene test tubes.

REAGENT PREPARATION


Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of 1x Wash Buffer.

sSortilin Standard - Reconstitute the sSortilin standard with 1.0 mL of **Dilution Buffer**. This reconstitution produces a stock solution of 200 ng/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making

dilutions. Pipette 250µL of Dilution Buffer into tubes #1 to #7. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The 200 ng/mL standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 ng/mL).

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
stock	Powder	1 ml	200 ng/ml
# 1	250µl of stock	250µl	100 ng/ml
# 2	250µl of 1	250µl	50 ng/ml
# 3	250µl of 2	250µl	25 ng/ml
# 4	250µl of 3	250µl	12.5 ng/ml
# 5	250µl of 4	250µl	6.25ng/ml
# 6	250µl of 5	250µl	3.125 ng/ml
# 7	250µl of 6	250µl	1.56 ng/ml

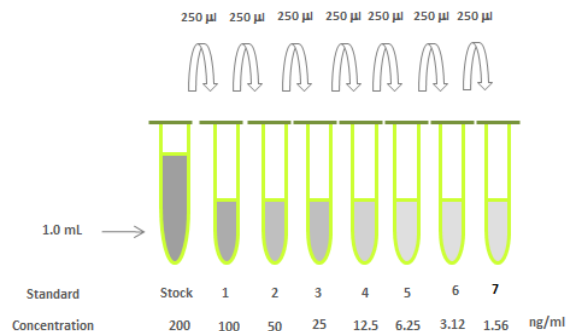

Positive Control - Reconstitute the Positive Control with 1.0 mL of **Dilution Buffer**. **Note:** Positive Control solution could be reused within a few days if stored at -20 °C or -70 °C.

Detection Antibody Concentrate – Reconstitute the Detection Antibody Concentrate with 1.05 mL of Dilution Buffer to prepare a 10-fold concentrated solution. Pipette 9.45 mL of **Dilution Buffer** into a 15 mL centrifuge tube and transfer the 1.05 mL of 10-fold concentrated solution to the tube to make 1x working solution.

Streptavidin-HRP Conjugate - Pipette 11.88 mL of **Dilution Buffer** into a 15 mL centrifuge tube and transfer 120 µL of 100-fold concentrated stock solution to prepare working solution. **Note:** 1x working solution of Streptavidin-HRP Conjugate should be used within a few days (**protect from light**).

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the plastic pouch (P01) with the desiccant pack.
3. Add 100µL per well of Dilution Buffer to Blank wells.
4. Add 100µL of standard dilutions in reverse order of serial dilution, sample, or positive per well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with 1x Wash Buffer (300µL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential for good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100µL of Detection Antibody working solution to each well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
7. Repeat the aspiration/wash as in step 5.
8. Add 100µL of Streptavidin-HRP Conjugate working solution to each well. Incubate for 1 hour on microplate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration/wash as in step 5.
10. Add 100µL of Substrate Solution to each well. Incubate 3-7 minutes on microplate shaker at room temperature. **Protect from light.**
11. Add 100µL of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a microplate reader set to 450nm.

CALCULATION OF RESULTS

Average the duplicate readings for each standard, positive control and sample, and subtract the average zero standard optical density. Create a

standard curve by reducing the data using computer software capable of generating a log-log curve fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the sSortilin concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

Calculation of samples with a concentration exceeding that of standard 200 ng/mL may result in inaccurate, low sSortilin levels. Such samples require further external pre-dilution according to expected sSortilin values with Dilution Buffer in order to precisely quantify the actual sSortilin level.

TYPICAL DATA

This standard curve is provided for demonstration only. A new standard curve should be generated for each set of samples assayed.

STANDARD (NG/ML)	CORRECTED (450NM)
Blank	0 (0.053)
1.56	0.090
3.125	0.169
6.25	0.298
12.5	0.539
25	0.871
50	1.264
100	1.631
200	2.171

- Lot No.:20111889
- Positive Control: 30 - 70 ng/mL

SPECIFICITY

PROTEIN NAME	CROSS-REACTIVITY
Mouse soluble Sortilin	100%
Mouse sCD36	0
Mouse sFNDC5	0
Mouse Endothelial lipase	0
Mouse sRAGE	0
Mouse VLP1	0

SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS
↓
Add 100 µl of standard dilutions, samples, or positive control to the well. Incubate 2 hours on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Detection Antibody working solution to each well. Incubate 2 hours on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Streptavidin-HRP conjugate working solution to each well. Incubate 1 hour on plate shaker at RT. Protect from light.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Substrate Solution to each well. Incubate 3-7 min on plate shaker at RT. Protect from light.
↓
Add 100 µl Stop Solution to each well. Read at 450nm within 15 min.